



LifeLink Tissue Bank Allograft Catalog



Your Global Link to the Future

*We Connect Healthcare
Professionals with a
World Class Tissue Bank*



We've helped surgeons and hospitals provide a multitude of second chances.

LifeLink is the largest not-for-profit tissue bank in the Southeastern United States providing more than 100,000 allografts each year to many surgical specialists. Over one million LifeLink allografts have been implanted since the tissue bank's inception. This amount is a direct result of our unwavering commitment to meeting or exceeding all FDA and industry standards.

It is our obligation to hospitals, surgeons and patients to provide the safest, highest quality allografts available. We accomplish this through a guiding conviction of respect, integrity, quality and safety.

For many people, an allograft transplant presents the opportunity to walk or run again, to live pain free and in some cases the chance to simply live a normal life.



To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org

Table of Contents



LifeGraft® Spinal Allograft.....	2
LifeFlex® Spinal Allograft	5
Sports Medicine Allograft.....	8
General Orthopedic Allograft.....	13
Wound Care	23
Quality	24
Hospital Services	25
Licenses and Certifications	26
Ordering and Customer Service.....	27
Packaging and Preservation.....	27
Procedures for Handling Freeze-Dried Allografts.....	28
Procedures for Handling Frozen Allograft	28
Transit and Storage Temperatures.....	28
Return Policies	29


LifeGraft® Spinal Allograft



*Our motto, **Safety From the Beginning®**, is the cornerstone of LifeLink's unparalleled quality assurance and control.*




LifeGraft® Spinal Allograft

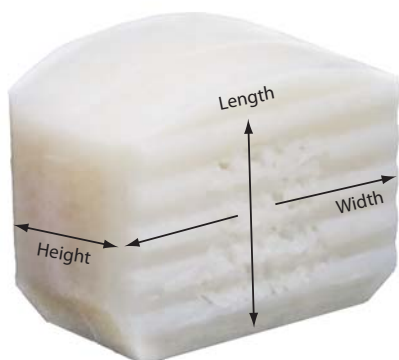

Cortical Cancellous Spacer

Dimensions			Catalog #	
Width	Length	Height	Freeze-Dried	
			Parallel	Lordotic
14.5mm	11.5mm	5mm	LGAP905	LGAL905
		6mm	LGAP906	LGAL906
		7mm	LGAP907	LGAL907
		8mm	LGAP908	LGAL908
		9mm	LGAP909	LGAL909
		10mm	-	LGAL910
14mm	14mm	6mm	-	LGAL956
		7mm	-	LGAL957
		8mm	-	LGAL958

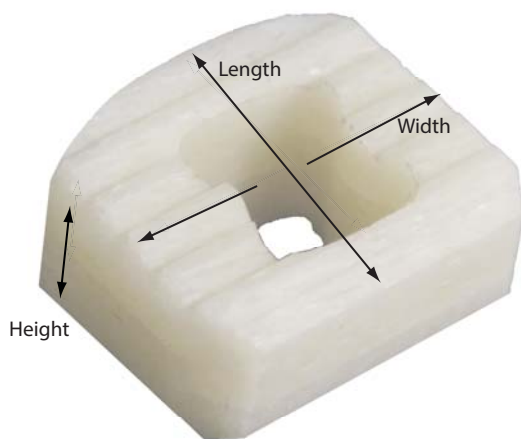

Cortical Spacer


Dimensions			Catalog #	
Width	Length	Height	Freeze-Dried	
			Parallel	Lordotic
14.5mm	11.5mm	5mm	LGAP915	LGAL915
		6mm	LGAP916	LGAL916
		7mm	LGAP917	LGAL917
		8mm	LGAP918	LGAL918
		9mm	LGAP919	LGAL919
		10mm	-	LGAL920
14mm	14mm	6mm	-	LGAL946
		7mm	-	LGAL947
		8mm	-	LGAL948



To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org


Tricortical Cancellous Wedge

Dimensions			Catalog #	
Width M/L	Length A/P	Height	Freeze-Dried	
			Parallel	Lordotic
13 - 15mm	13 - 15mm	5mm	LGAP705	LGAL705
		6mm	LGAP706	LGAL706
		7mm	LGAP707	LGAL707
		8mm	LGAP708	LGAL708
		9mm	LGAP709	LGAL709
		10mm	LGAP710	LGAL710

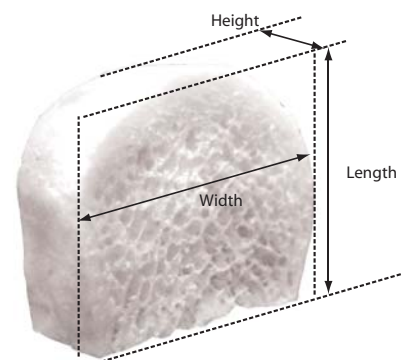


Unicortical Cancellous Spacer

Dimensions			Catalog #
Width	Length	Height	Parallel/Freeze-Dried
14mm	11mm	5mm	LGAP505
		6mm	LGAP506
		7mm	LGAP507
		8mm	LGAP508
		9mm	LGAP509
		10mm	LGAP510

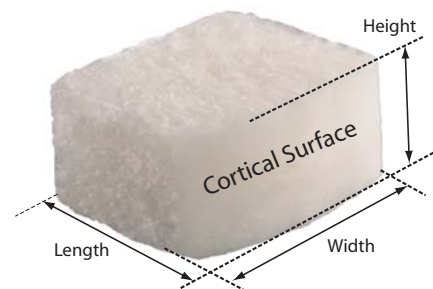


To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org

LifeFlex® Spinal Allograft

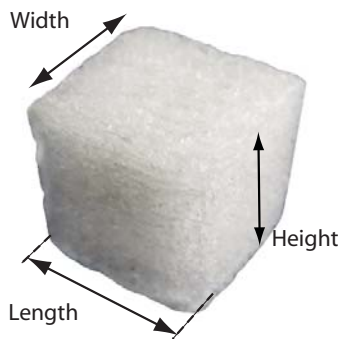

LifeFlex® Demineralized Cancellous Cube

Specifications			Catalog #
Height	Width	Length	Freeze-Dried
8mm	8mm	8mm	15A008
10mm	10mm	10mm	15A010
12mm	12mm	12mm	15A012
14mm	14mm	14mm	15A014

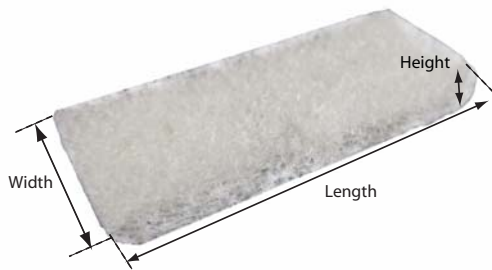

LifeFlex® Demineralized Cancellous Strip

Specifications			Catalog #
Height	Width	Length	Freeze-Dried
5mm	15mm	50mm	15A035
5mm	20mm	50mm	15A040
8mm	25mm	50mm	15A050



LifeFlex® Demineralized Cortical Fibers

Specifications	Catalog #
	Freeze-Dried
5cc	17A105
10cc	17A110
15cc	17A115



To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org

Spinal Contract Allograft



Indux™ Cancellous Strip

Dimensions	Catalog #
	Freeze-Dried
5 x 20 x 50mm	45-3250
8 x 25 x 50mm	45-3208

Tissue represented by Zimmer Biomet Spine, Inc. To place an order call 800-348-2759



Osteoamp® Compressible Sponge Strip

Dimensions	Catalog #
	Freeze-Dried
7 x 10 x 50mm, Large	13812209
7 x 20 x 50mm, XL	13812509

Tissue represented by Bioventus Surgical. To place an order call 800-637-4391



SiJoin Sacroiliac Joint Fusion Implant

Dimensions	Catalog #
	Freeze-Dried
6 x 11 x 15mm	VG-SJ-AG-11511
6 x 11 x 20mm	VG-SJ-AG-TS-12011

Tissue represented by VGI Medical, LLC. To place an order call 727-565-1235



NuFix® I Cortical Dowel

Dimensions	Catalog #
	Freeze-Dried
5.0 x 9mm	10050
5.5 x 9mm	10055

Tissue represented by Nutech Spine. To place an order call 205-329-7285

Spinal Contract Allograft



NuFix® II Cortical Dowel

Dimensions	Catalog #
	Freeze-Dried
5.0 x 10 x 10.5mm	20050

Tissue represented by Nutech Spine. To place an order call 205-329-7285



SIFix® Intra-Articular Fusion Allograft (Cancellous)

Dimensions	Catalog #
	Freeze-Dried
11 x 22mm	1743011

Tissue represented by Nutech Spine. To place an order call 205-329-7285



SIFix® Intra-Articular Fusion Allograft (Cortical)

Dimensions	Catalog #
	Frozen
11 x 22mm	3743011

Tissue represented by Nutech Spine. To place an order call 205-329-7285




Sports Medicine Allograft

LifeLink goes to great lengths to ensure the safety of our allograft bone and tissue.

LifeLink®




Tissue Bank

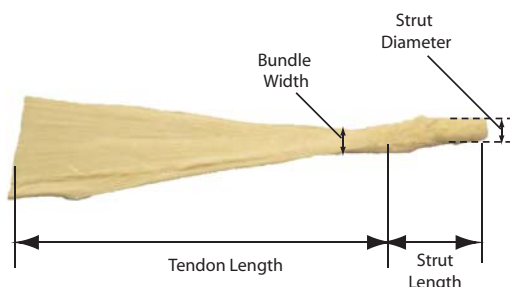


Achilles Tendon Preshaped

Specifications				Catalog #	
	Diameter	Width	Length	Aseptically Processed	Gamma Irradiated
Strut	10mm	-	25mm min.	02B003	50R102
Tendon	-	-	160mm min.		
Bundle	-	Measure	-		

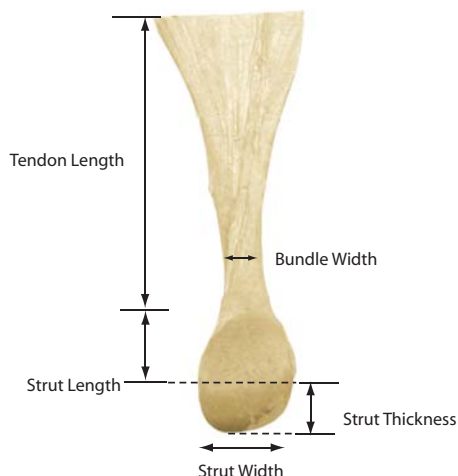

Achilles Tendon with Strut

Specifications				Catalog #	
	Diameter	Width	Length	Aseptically Processed	Gamma Irradiated
Strut	Measure	12mm min.	25mm min.	02B002	50R103
Tendon	-	-	160mm min.		
Bundle	-	Measure	-		

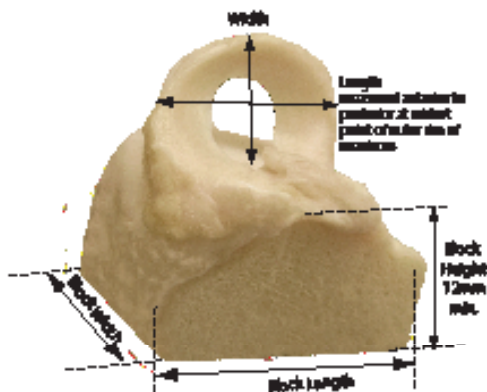


Meniscus Half

Specifications		Catalog #	
Graft	Size	Aseptically Processed	Patient Matched Aseptically Processed
Left Medial	Measure	90B007-X	90B007
Left Lateral	Measure	90B008-X	90B008
Right Medial	Measure	90B010-X	90B010
Right Lateral	Measure	90B011-X	90B011

 To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org


Patella Tendon Preshaped

Specifications				Catalog #	
Struts		Tendon		Aseptically Processed	Gamma Irradiated
Diameter	Length	Width	Length		
10mm	25mm min.	10mm min.	30 - 50mm	47B010	50R301

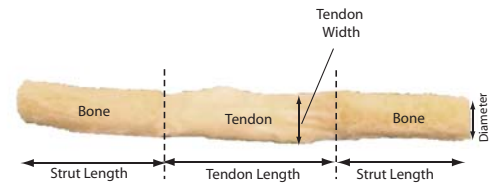


Patella Tendon with Strut- Half

Specifications					Catalog #	
	Thickness	Width	Length		Aseptically Processed	Gamma Irradiated
Tendon	-	10mm min.	To Strut	To Attachment	46B002	50R302
			Measure	35-45mm min.		
Struts	12mm min.	10mm min.	25mm min.			

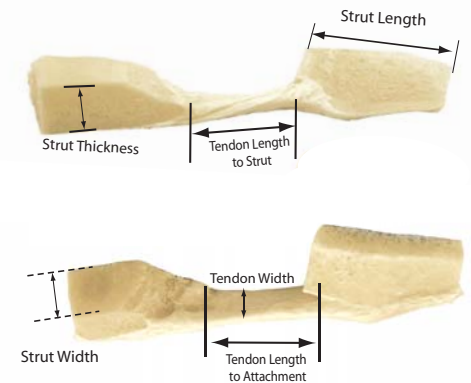

Patella Tendon with Strut- Whole

Specifications					Catalog #	
	Thickness	Width	Length		Aseptically Processed	Gamma Irradiated
Tendon	-	15mm min.	To top of Strut	To Attachment	46B005	50R303
			Measure	35-45mm min.		
Struts	15mm min.	15mm min.	25mm min.			
w/ Quad	-	-	50mm min.		46B006	50R304

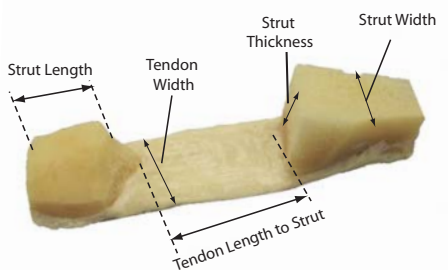

Sports Medicine Allograft




Patella Tendon w/Extensor Mechanism

Specifications				Catalog #
	Thickness	Width	Length	Aseptically Processed
Quad Tendon	-	-	120mm min.	46B020
Patella Tendon	-	Measure	35mm min. to attachment	
Tibial Strut	25mm min.	25mm min.	100mm min.	


Peroneus Longus Tendon

Dimensions			Catalog #	
Diameter	Width	Length	Aseptically Processed	Gamma Irradiated
8mm min. (Folded)*	Measure (Single strand)	240mm min.	81B006	50R401



Semitendinosus/Gracilis


Dimensions			Catalog #		
Diameter	Width	Minimum Length	Allograft Type	Aseptically Processed	Gamma Irradiated
4mm min. (Folded)*	Measure (Single strand)	200mm	Semitendinosus	81B003	50R502
3mm min. (Folded)*	Measure (Single strand)	200mm	Gracilis	81B004	50R501
8mm min. (Folded)*	-	200mm	Semitendinosus with Gracilis	81B005	50R503

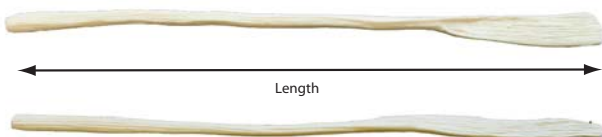


To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org

Tibialis Tendon



Dimensions				Catalog #	
Diameter	Width	Length	Allograft Type	Aseptically Processed	Gamma Irradiated
8mm min. (Folded)*	Measure (Single strand)	240mm min.	Anterior	81B001	50R601
			Posterior	81B002	50R602



How we measure our soft tissue allografts

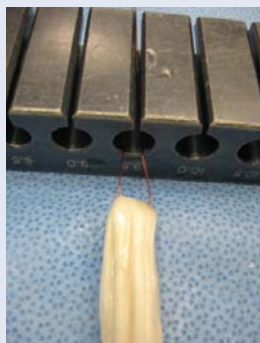

*The diameter is determined by pulling the folded tendon through the appropriate channel of the sizing block smoothly and without excessive force.

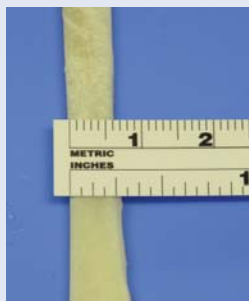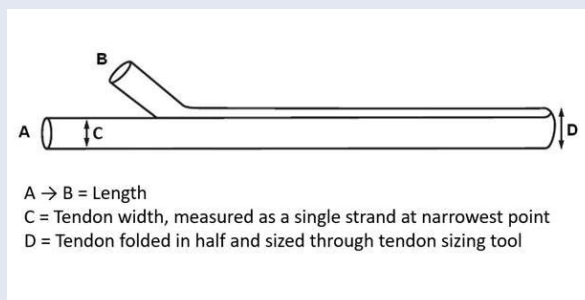

General Orthopedic Allograft





Our continuous focus on service ensures that surgeons receive the allografts they need when they need them.

LifeLink[®]

Tissue Bank

General Orthopedic Allograft

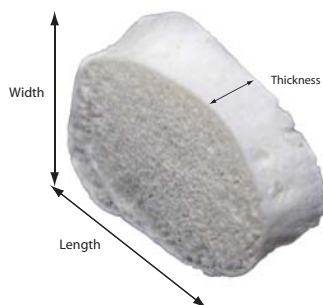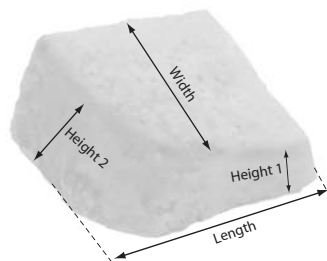

Bicortical Foot Wedge

Specifications					Catalog #
	Height 1	Height 2	Width	Length	Freeze-Dried
6mm COTTON	2.5mm	6mm	14mm	24mm	67A006
8mm EVANS	3.5mm	8mm	22mm	20mm	67A008
10mm EVANS	5.5mm	10mm	22mm	20mm	67A010
12mm EVANS	7.5mm	12mm	22mm	20mm	67A012

Bone Plug

Specifications		Catalog #
Diameter	Length	Freeze-Dried
12mm	18 mm min. - 25mm max.	03A003
13mm	18 mm min. - 25mm max.	03A006
14mm	18 mm min. - 25mm max.	03A004
16mm	18 mm min. - 25mm max.	03A005

Calcaneus Wedge

Specifications			Catalog #
Thickness	Width	Length	Freeze-Dried
10mm	30mm min.	40mm min.	04A002

Cancellous 1-4mm

Specifications	Catalog #	
	Freeze-Dried	Frozen
5cc	05A101	05B101
15cc	05A001	05B005
30cc	05A002	05B006
60cc	05A008	05B009
90cc	05A010	05B007

 To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org

General Orthopedic Allograft

Cancellous 4-10mm

Specifications	Catalog #	
	Freeze-Dried	Frozen
5cc	08A024	-
15cc	08A022	08B023
30cc	08A020	08B024
60cc	08A021	08B025
90cc	08A023	-




Cancellous 250-850µm

Specifications	Catalog #
	Freeze-Dried
15cc	07A001
30cc	07A004



Cancellous Block

Dimensions			Catalog #
Thickness	Width	Length	Freeze-Dried
20mm	20mm	40mm	09A004

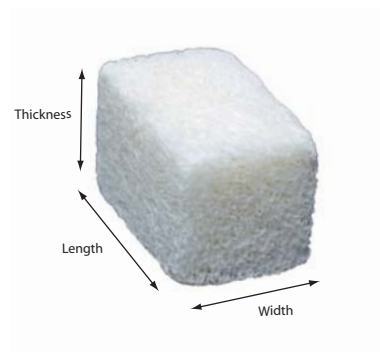

Cancellous Cortical 1-4mm

Specifications	Catalog #
	Freeze-Dried
15cc	10A002
30cc	10A001



 To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org

General Orthopedic Allograft



Cancellous Cortical 4-10mm

Specifications	Catalog #
	Freeze-Dried
15cc	19A002
30cc	19A001

Cancellous Cortical Matchsticks



Specifications			Catalog #	
	Width	Length	Quantity	Freeze-Dried
Small	3 - 6mm	60mm	3 / Pack	18A008
			6 / Pack	18A006
Large	3 - 6mm	80mm	3 / Pack	18A009
			6 / Pack	18A005

Cancellous Cubes

Dimensions			Catalog #	
Thickness	Width	Length	Freeze-Dried	
10mm	10mm	10mm	13A001	4 pack
10mm	10mm	10mm	13A002	1 pack

Cortical Segment

Specifications			Catalog #	
	Width	Length	Freeze-Dried	Frozen
Small	Measure	40 - 65mm	71A003	71B004
Large	Measure	66 - 99mm	71A004	71B005

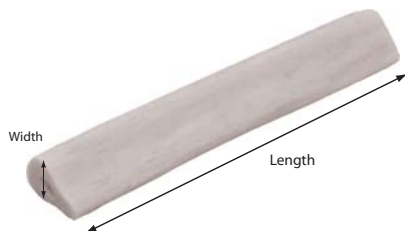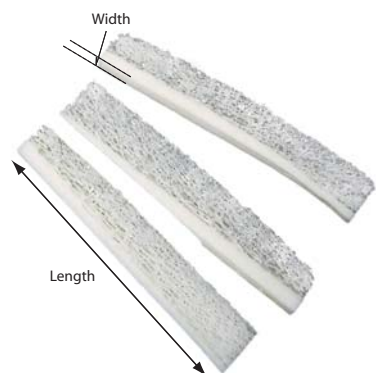


To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org

General Orthopedic Allograft


Cortical Shaft

Specifications			Catalog #	
	Width	Length	Freeze-Dried	Frozen
Small	Measure	100 - 125mm	72A002	72B005
Large	Measure	126mm min.	72A003	72B006

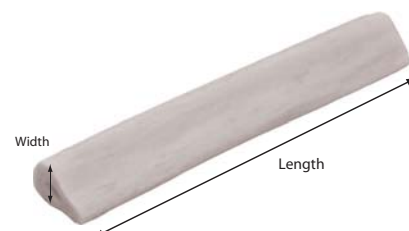

Costal Cartilage


Dimensions		Catalog #
Width	Length	Frozen
10mm min.	30mm min.	70B001

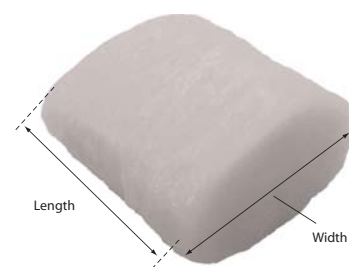


Fascia

Dimensions		Catalog #
Width	Length	Freeze-Dried
60mm min.	140mm min.	21A001

Dimensions		Catalog #
Width	Length	Frozen
80mm	80mm	21B007

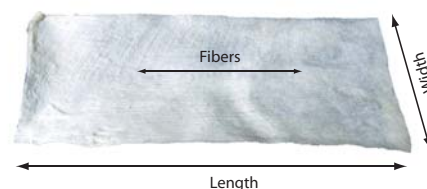


General Orthopedic Allograft

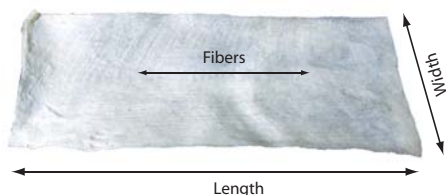

Fascia Strip

Dimensions		Catalog #
Width	Length	Freeze-Dried
40 - 60mm	50 - 140mm	21A005

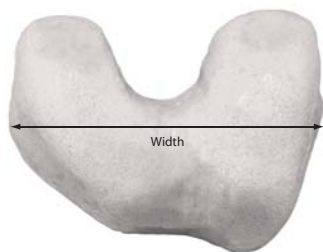

Femur Condyle

Specifications		Catalog #	
Width		Freeze-Dried	Frozen
Measure Medial to Lateral	Whole	22A003	22B004
	Half	22A001	22B002



Femur Head

Specifications	Catalog #	
Diameter	Freeze-Dried	Frozen
40mm min.	24A001	24B002


 To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org

General Orthopedic Allograft

Femur Plate

Specifications		Catalog #	
Width*	Length	Freeze-Dried	Frozen
20mm min.	150mm min.	25A001	25B003

*Width is measured on smallest end of shaft

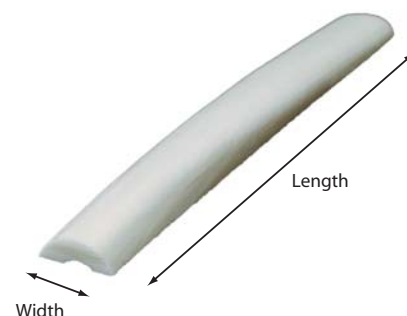


Femur Shaft

Specifications		Catalog #	
Width	Length	Freeze-Dried	Frozen
25mm min.	150mm min.	27A005	27B006




HTO Wedge

Specifications					Catalog #
Description	Height 1 +0 / -2.0mm	Width	Length	Height 2	Freeze-Dried
HTO Wedge 6°	7.5mm	Measure	Measure 35mm min. 50mm max.	Measure 3mm min.	64A106
HTO Wedge 8°	10.0mm	Measure			64A108
HTO Wedge 10°	12.5mm	Measure			64A110
HTO Wedge 12°	15.0mm	Measure			64A112
HTO Wedge 14°	17.5mm	Measure			64A114

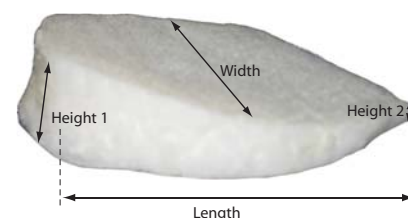

 To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org

General Orthopedic Allograft



Humerus Head


Specifications	Catalog #	
Diameter	Freeze-Dried	Frozen
40mm min.	34A001	34B002



Humerus Shaft


Specifications		Catalog #	
Width*	Length	Freeze-Dried	Frozen
15mm min.	100mm min.	37A002	37B003

*Width is measured on smallest end of shaft

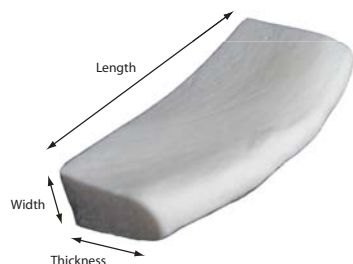

Iliac Crest Strip

Specifications			Catalog #
Thickness	Width	Length	Freeze-Dried
15mm min.	9mm min.	50 - 80mm	40A003

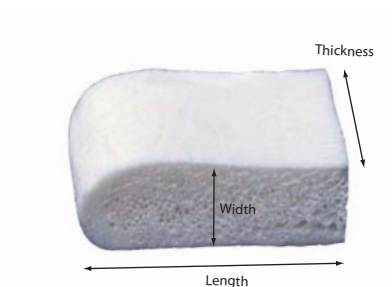

Iliac Crest Wedge

Specifications				Catalog #	
	Thickness	Width	Length*	Freeze-Dried	Frozen
Sm.	7mm min. 14mm max.	9mm min.	18mm min. 25mm max.	40A002	N/A
Lg.	15mm min. 25mm max.	10mm min.	25mm min. 30mm max.	40A001	40B004

*No more than 3mm variance on length from side to side




To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org

General Orthopedic Allograft

Ilium Block Tricortical


Specifications			Catalog #
Thickness	Width	Length	Freeze-Dried
15mm min. 25mm max.	20mm min.	75mm min.	39A002

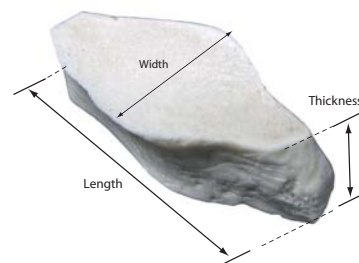

Ilium Strip Tricortical


Specifications			Catalog #
Thickness	Width*	Length	Freeze-Dried
15mm min. 25mm max.	10mm min.	65mm min.	42A001

*Width is measured at centerline of graft

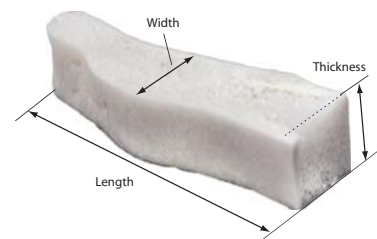


Patella Wedge

Specifications			Catalog #
Thickness	Width	Length	Freeze-Dried
15mm min.	13mm min.	30mm min.	46A005

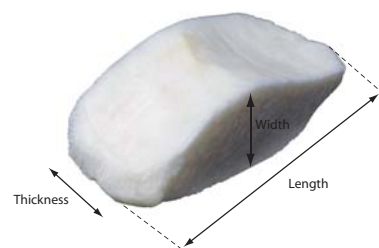


 To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org

General Orthopedic Allograft

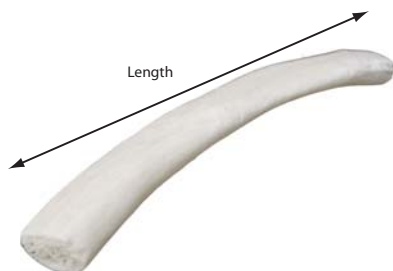

Rib Whole

Specifications	Catalog #
Length	Freeze-Dried
80mm min.	51A001

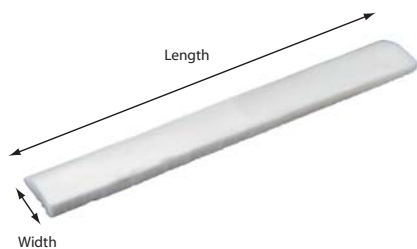

Tibia Plate

Specifications		Catalog #	
Width	Length	Freeze-Dried	Frozen
20mm min. – 30mm max.	150mm min.	56A001	56B002



Tibia Shaft

Specifications		Catalog #	
Width*	Length	Freeze-Dried	Frozen
Measure	150mm min.	59A002	59B003

*Width is measured on smallest end of shaft



To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org

Wound Care

Affinity Fresh Amniotic Membrane

Specifications		Catalog #
Width	Length	
1.5 cm	1.5 cm	AF-1150
2.5 cm	2.5 cm	AF-1250

Tissue represented by Organogenesis. To place an order call 800-824-9194



Our formula for success is immensely effective: Safety from the Beginning®

A full service tissue bank since 1985, LifeLink ensures that all established state and federal requirements and AATB Standards for recovery, processing, packaging and distribution of human allograft tissue are met. Our motto, *Safety From The Beginning®*, is the cornerstone of LifeLink's unparalleled quality assurance and control. From using donor screening criteria that is among the most stringent in the nation, to processing all tissue in ISO-classified cleanrooms, we have earned a reputation in the medical community for providing allografts of unsurpassed safety and quality.

The following are a few of the LifeLink standards:

- Our tissue is recovered under strict aseptic conditions within our three Federally designated OPO service areas or from tissue recovery partners qualified by LifeLink to meet AATB Standards for Tissue Banking.
- All LifeLink musculoskeletal tissue is processed using Allowash® technology. While most of our grafts receive low dose gamma irradiation, the majority of sports and demineralized allografts are non-irradiated.
- On-site CAP accredited microbiology laboratory helps ensure quality throughout the process, by handling pre-processing, in-process, and release testing (as applicable).
- Medical Directors available to tissue bank staff and medical screening personnel 24 hours a day, 7 days a week, 365 days a year.



Pre-processing microbial cultures are collected on all tissue at the time of recovery and all aseptically processed batches of final allografts undergo destructive testing

LifeLink goes to great lengths to ensure the safety of our allografts. In addition to evaluating the donor's medical and social history, relevant medical records and autopsy (if performed), infectious disease testing is performed. All tissue is determined to be suitable for transplantation after a thorough review of these items by a LifeLink Tissue Bank Medical Director. Destructive testing is performed on each batch of aseptically processed tissue to detect the presence of microorganisms, or the tissue is terminally sterilized using gamma radiation. As a final safety measure, all processing documentation is reviewed by the Quality Control team to ensure all quality requirements have been met.

Donor infectious disease testing includes the following:

- HIV1/HIV2 AB (Plus O) ■ HBsAg ■ HBcAb ■ HCVAb
- HIV1/HCV/HBV NAT ■ STS (Serologic Test for Syphilis)

Hospital Services

Our continuous focus on service ensures that surgeons receive the allografts they need when they need them.

Life changing allografts are of no use if they are not in the right place at the right time, delivered into a physician's hands. Understanding the timely importance of this process, LifeLink's highly trained customer service team is ready to respond 24/7, 365 days a year.

- Staff members are highly knowledgeable of allograft tissue and their numerous surgical applications
- We are available to assist your hospital and surgeons with technical support, cost containment strategies and graft selection
- We can assist with consignment and inventory management
- We will work with your hospital to ensure that surgeons' allograft needs are fulfilled
- We support hospitals with Joint Commission compliance inspections and can provide continuing education opportunities
- Service is available 24 hours a day, 7 days a week, 365 days a year



Emergency Requests:

- Staff is available 24 hours a day to handle any emergency
- Overnight express delivery is utilized for out-of-town orders
- Same day delivery arrangements are made for local emergency orders

Consignment Program:

- Wide range of grafts constantly available in the OR
- Hospital pays for allografts only after implantation
- Hospital does not bear loss from expired allografts
- Shipping, handling and restocking fees are eliminated on consigned allografts, including returns



To place an order call 1-800-683-2400 or email hs.orders@lifelinkfound.org

Licenses and Certifications



LifeLink's ultimate goal is to preserve and improve a patient's quality of life.

LifeLink Tissue Bank is a division of the LifeLink Foundation, an independent not-for-profit organization, dedicated to the recovery and transplantation of organs and tissue. Since 1982, the Foundation has worked in a sensitive, diligent and compassionate manner to help save and improve lives. LifeLink Foundation consists of five divisions, which includes the tissue bank, three organ procurement organizations, and an immunology laboratory.

Licenses and Certifications

- LifeLink Tissue Bank is accredited by the American Association of Tissue Banks
- Registered with the FDA
- Registered with Health Canada
- Licensed by the States of Florida, California, and New York
- Holds a permit to distribute in Maryland and is registered in Delaware, Oregon and Illinois

Copies of LifeLink Tissue Bank's current licenses and accreditations can be obtained at <https://www.lifelinktissuebank.org/health-professionals/certifications/>

Ordering LifeLink Allografts



LifeLink's Hospital Services department is available to answer questions and process requests Monday through Friday from 8:00 a.m. until 5:00 p.m. EST. On-call service is also available for emergencies after hours. Staff is available 24 hours a day, 7 days a week, 365 days a year.

Advanced ordering is recommended to ensure prompt delivery. A purchase order number is always required prior to shipment to effectively process an order.



To place an order call **1-800-683-2400** or email hs.orders@lifelinkfound.org

Shipping

All local orders are handled by an established courier service or FedEx. We utilize FedEx Priority for all orders outside the LifeLink service area. Same day delivery arrangements are made for emergency orders.

Packaging and Preservation

State-of-the-art techniques are utilized to package and preserve tissue. All packaging is completed in continuously monitored cleanrooms and placed in double heat sealed Tyvek® envelopes. Allografts are then preserved utilizing one of the following commonly accepted methods:

- **Freeze-drying or lyophilization:** This is the most commonly applied preservation method for tissues. Specific freeze-drying cycles are utilized to ensure a residual moisture level of 6% or less.
- **Freezing:** A method in which allograft tissue is packaged and then stored at -40 degrees celsius or colder.

Recommended Procedure for Handling and Reconstitution of Freeze-Dried Allografts

Freeze-dried allografts are stored at ambient temperature (11°C-25°C; 52°F-77°F). Rehydration time varies with the type of allograft. Freeze-dried weight bearing bone allografts that are to be sawed, drilled, or shaped should be rehydrated to ensure that the tissue will not be brittle. If the allograft is to be rehydrated longer than two hours, it should be refrigerated until use. Smaller non-weight bearing bone allografts generally do not require rehydration.

Once removed from the package, the allograft should be implanted immediately or refrigerated and used within 24 hours (if stored with proper precautions to prevent contamination).

Please refer to package insert for detailed instructions.

Recommended Procedure for Thawing Frozen Allografts

To prepare the allograft for use, it must be thawed. Thawing time for most frozen allografts is about 15-30 minutes at room temperature. For larger structural grafts, thaw for up to one hour. Soft tissue allografts must be thawed until they become soft and pliable.

Once thawed, the allograft should be implanted immediately or refrigerated and used within 24 hours (from start of thawing) if stored with proper precautions to prevent contamination.

Please refer to package insert for detailed instructions.

Transit and Storage Temperatures

Frozen allografts are shipped to the hospital on dry ice and should be stored at -40° Celsius or colder until use. Temperatures between -20° Celsius and -40° Celsius are acceptable for short-term storage (six months or less). For returns however, LifeLink only accepts frozen tissue that has been stored at -40° Celsius or colder. Unless it is being thawed for implantation, a graft removed from the freezer should be maintained in a transport container with dry ice completely surrounding the allograft. The time the graft is removed from and returned to the freezer should be documented in the Allograft Management Log. Care should be taken when working with dry ice, as burns may result from contact with unprotected skin.

Freeze-dried allografts do not have a specific required environmental temperature during shipping and are shipped at ambient temperature. Upon receipt, freeze-dried allografts should be stored at ambient temperature (11°-25°C; 52°F-77°F).

The methods of processing and storage utilized by LifeLink Tissue Bank are well documented and have been proven effective by many years of clinical experience.

Tracking

Traceability of each allograft is maintained by means of an automated system. Each allograft is assigned a unique identifying number that allows complete traceability from the donor through each stage in processing, storage and shipment to the end user. Included with each packaged allograft is an Allograft Implant Record which must be completed and returned to LifeLink Tissue Bank upon implantation. This information is essential for maintaining a complete record of all allografts shipped from LifeLink Tissue Bank.

Returns

- Return Authorization will only be issued for Frozen or Freeze Dried allografts that meet the criteria for return
- All returns must be pre-authorized by LifeLink Tissue Bank's Hospital Services Department

For detailed information about returning allograft, to obtain return authorization, or to report a complication, please contact the LifeLink Tissue Bank Hospital Services department at 800-683-2400 or email HS.Orders@lifelinkfound.org



Hospital Services

LifeLink Tissue Bank
9661 Delaney Creek Blvd.
Tampa, Florida 33619

Toll Free 800-683-2400

Local 813-886-8111

Fax 813-886-1851

www.lifelinktissuebank.org